

# NBL-WQ-OIL-4S Online Water Oil Sensor User Manual



Changsha Zoko Link Technology Co., Ltd.

Tel:+8615367865107

E-mail: [sales@niubol.com](mailto:sales@niubol.com)

Website: [www.niubol.com](http://www.niubol.com)

Address: Room 102, District D, Houhu Industrial Park, Yuelu District, Changsha City,

Hunan Province, China

## User Notes

- Please read the instruction carefully before using and save it for reference.
- Please follow the instructions and precautions.
- When receiving the instrument, please open the packaging carefully, inspect equipment's damage level in case of transportation, if you found spoiled equipment, please immediately notify the manufacturer and distributor, and retain the packaging, in order to send back to processing.
- When the instrument is in trouble, please don't repair it by yourself, please directly contact the maintenance department of the manufacturer.

# Content

I 、 Working principle .....	4
II 、 Technical performance and specifications .....	4
1. Technical parameters .....	4
2. Dimensional drawing .....	5
III、 Installation and electrical connection .....	5
1. Installation .....	5
2. Electrical connection .....	5
IV、 Maintenance .....	6
1. Maintenance procedures and methods .....	6
2. Sensor calibration .....	6
3. Frequently asked questions .....	6
V 、 Quality and service .....	7
1. Quality assurance .....	7
2. Accessories and spare parts .....	7
3. After-sales service commitment .....	7
Appendix data communication .....	8

## I 、 Working principle

Integrated water Oil sensor is the use of soluble oil absorption peaks in spectra and emission peak of the properties, in the spectrum of soluble oil absorption peak emission monochromatic light exposure to water, soluble oil absorb light energy, releasing another emission peak wavelength of monochromatic light, soluble oil emission intensity is proportional to the content of water soluble oil. The sensor is easy to install and use.

- UV LED light source, high stability, long service life, small drift
- Ac driven, effectively filter natural light interference
- Support RS-485 (Modbus/RTU protocol)
- Convenient, fast, stable and easy to maintain


## II 、 Technical performance and specifications

### 1. Technical parameters

<b>Model</b>	NBL-WQ-OIL-4S
<b>Measuring range</b>	0~40.00mg/L
<b>Resolution</b>	0.01mg/L
<b>Accuracy</b>	±3%
<b>Calibration</b>	Two-point calibration
<b>Protection grade</b>	IP68
<b>Working conditions</b>	0~50℃, <0.2MPa
<b>Storage temperature</b>	-5~65℃
<b>Sensor interface</b>	RS-485(Modbus/RTU) 、 4-20mA(Optional)
<b>Power information</b>	12~24VDC
<b>Power consumption</b>	0.2W@12V

<b>Cable length</b>	5 meters, other lengths can be customized
<b>Shell material</b>	ABS and 316L stainless steel

## 2. Dimensional drawing

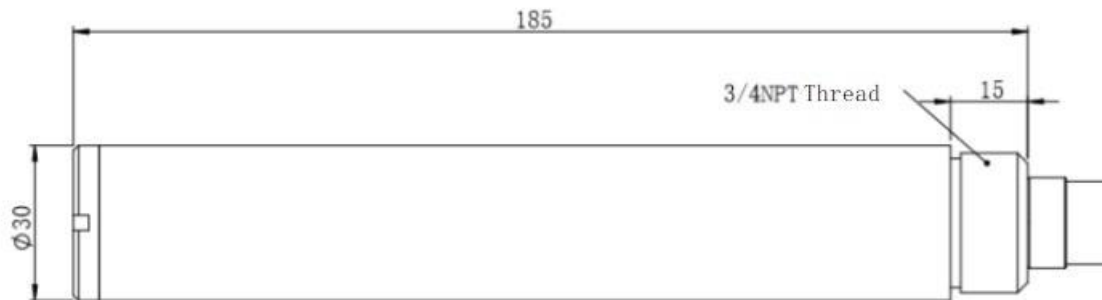

**Note:** The sensor connector is the male end of M16-5 core waterproof connector.

## III、 Installation and electrical connection

### 1. Installation

Installation distance requirement: keep more than 2cm with the side wall and 10cm or more with the bottom.

### 2. Electrical connection

The cable is 5-core twisted pair shielded wire, the wire sequence definition:

- Red cord—power cord (12V~24VDC)
- Black cord —ground cord (GND)
- Blue cord—485A
- Green cord—485B
- Yellow cord—Current output (if unused, suspended)

The wiring sequence should be carefully checked before power-on to avoid unnecessary losses caused by faulty wiring.

**Wiring instructions:** considering the cable long-term Immersion in water (including sea water) or exposure to air, all wiring are required to do waterproof treatment, the user cable should have a certain degree of corrosion resistance.

## IV、 Maintenance

### 1. Maintenance procedures and methods

#### 1.1 Maintenance schedule

The cleanliness of the measurement window is very important to maintain accurate readings.

Maintenance task	Recommended maintenance frequency
Calibrate the sensor (if required by the competent authority)	According to the maintenance schedule required by the competent authority

### 1.2 Maintenance methods

- Sensor outer surface: Clean the outer surface of the sensor with tap water. If there is still debris left, wipe it with a soft, damp cloth. For some stubborn dirt, add some household washing liquid to the tap water to clean it.
- Check the cable of the sensor: the cable should not be tightened during normal operation. Otherwise, the internal cable of the cable may be broken and the sensor may not work normally.
- Check the sensor's measurement window for dirt.

### 1.3 Precautions

The probe contains sensitive optical and electronic components. Make sure the probe is not subject to severe mechanical shock. There are no parts inside the probe that require user maintenance.

## 2. Sensor calibration

a) Zero calibration: Take a proper amount of distilled water in a large bucket and place the sensor vertically in the solution. The front end of the sensor is at least 10 cm away from the bottom of the beaker. After 3 to 5 minutes, the value is stabilized and the zero point is calibrated. The instructions refer to the appendix.

b) Slope calibration: Place the sensor probe in the standard solution. The front end of the sensor is at least 10cm away from the bottom of the beaker. After 3 to 5 minutes, the slope is calibrated after the value is stable. The instructions refer to the appendix.

## 3. Frequently asked questions

Problem	Possible reason	Solution
The operation interface cannot be connected or the measurement result is not displayed.	The measured value is too high, too low or the value is continuously unstable	Reconnect controller and cable
	Cable failure	Please contact us
The measured value is too high, too low or the value is continuously unstable	The sensor window is attached by a foreign object	Cleaning the sensor window surface

## V 、 Quality and service

### 1. Quality assurance

- The quality inspection department has standardized inspection procedures, advanced and perfect testing equipment and means, and strictly in accordance with the regulations, to do 72-hour aging test and stability test on the product, and not to allow one unqualified product to leave the factory.
- The receiving party directly returns the product batch with a failure rate of 2%, and all the costs incurred are borne by the supplier. The reference standard refers to the product description provided by the supplier.
- Guarantee the quantity of goods and the speed of shipment.

### 2. Accessories spare and parts

This product includes:

- 1 sensor
- 1 copy of the manual
- 1 certificate
- 1 Cable (5 m)

### 3. After-sales service commitment

The company provides local after-sales service within one year from the date of sale, but does not include damage caused by improper use. If repair or adjustment is required, please return it, but the shipping cost must be conceited. Damaged on the way, the company will repair the damage of the instrument for free.

## Appendix data communication

### 1. Data format

The default data format for Modbus communication is: 9600, n, 8, 1 (baud rate 9600bps, 1 start bit, 8 data bits, no parity, 1 stop bit).

Parameters such as baud rate can be customized.

### 2. Information frame format

a) read data instruction frame

0F	03	xx xx	xx xx	xx xx
Address	Function code	Register address	Number of registers	CRC check code (low byte first)

b) read data response frame

0F	03	xx	xx.....xx	xx xx
Address	Function code	Bytes	Answer data	CRC check code (low byte first)

c) write data instruction frame

0F	06	xx xx	xx xx	xx xx
Address	Function code	Register address	Write data	CRC check code(low byte first)

d) Write data response frame (same data command frame)

0F	06	xx xx	xx xx	xx xx
Address	Function code	Register address	Write data	CRC check code (low byte first)

### 3. Register address

Register address	Name	Instruction	Number of registers	Access method
40001 (0x0000)	Value	Two double-byte integers, which are measured values and measured decimal places.	2 ( 4 bytes )	Read

44097 (0x1000)	Zero calibration	Calibrated in distillation, the write data is 0; the read data is zero offset. (It can also be calibrated in a standard solution of 0-10ppm. The calibration method is based on the slope calibration)	1 ( 2 bytes )	Write/Read
44101 (0x1004)	Slope calibration	Calibrate in the known standard solution (10ppm -- 40ppm), and write data as the actual value of the standard solution $\times 100$ ; The read data is the slope value $\times 1000$ .	1 ( 2 bytes )	Write/Read
48195 (0x2002)	Device address	Default is 15. Write data range 1-255.	1 ( 2 bytes )	Write/Read
48225 (0x2020)	Factory reset	The calibration value restores the default value and the write data is 0. Note that the sensor must be recalibrated before use after reset.	1 ( 2 bytes )	Write

#### 4. Command example

a) Start measurement command

Function: Get the oil value in the water measured by the sensor; the unit of oil in the water is mg/L.

Request frame: 0F 03 00 00 00 02 C5 25

Response frame: 0F 03 04 01 02 00 02 34 0E

Reading example:

Oil value in water
01 02 00 02

For example: the value of oil in water 01 02 represents the value of oil in water in hexadecimal reading, 00 02 represents the value of oil in water with 2 decimal points, and the converted decimal value is 2.58.

b) Calibration instructions

Zero point calibration

Function: Set the zero point calibration value of the oil in the sensor water; here the zero point

calibration is performed in distilled water;

Request frame: 0F 06 10 00 00 00 8C 24

Response frame: 0F 06 10 00 00 00 8C 24

slope calibration

Function: Set the slope calibration value of the sensor's oil in water; the slope value here is based on the actual standard solution value x100. Take 30 mg/L as an example to refer to the calibration;

Request frame: 0F 06 10 04 0B B8 CA A7

Response frame: 0F 06 10 04 0B B8 CA A7

c) Set device ID address:

Function: Set the Modbus device address of the sensor;

Change the sensor address 0F to 01, the example is as follows

Request frame: 0F 06 20 02 00 01 E3 24

Response frame: 0F 06 20 02 00 01 E3 24

## 5. Error respond

If the sensor does not correctly execute the host command, it will return the following format information:

Definition	Address	Function code	Code	CRC check
Data	ADDR	COM+80H	xx	CRC 16
Number of bytes	1	1	1	2

a) CODE: 01 –Function code error

03 – Data is wrong

a) COM: The received function code